

Accepted refereed manuscript of:

Jääskeläinen AJ, Sironen T, Diagne CT, Diagne MM, Faye M, Faye O, Faye O, Hewson R, Mölsä M, Weidmann MW, Watson R, Sall AA & Vapalahti O (2019) Development, validation and clinical evaluation of a broad-range pan-filovirus RT-qPCR. *Journal of Clinical Virology*, 114, pp. 26-31.

DOI: <https://doi.org/10.1016/j.jcv.2019.03.010>

© 2019, Elsevier. Licensed under the Creative Commons Attribution-NonCommercial-NoDerivatives 4.0 International

<http://creativecommons.org/licenses/by-nc-nd/4.0/>

Abstract

Background

During the five decades since their discovery, filoviruses of four species have caused human hemorrhagic fever outbreaks: Marburg (MARV) marburgvirus, and Zaire (EBOV), Sudan (SUDV) and Bundybugyo (BDBV) ebolaviruses. The largest, devastating EBOV epidemic in West Africa in 2014-16, has been followed by outbreaks of MARV in Uganda, 2017, and EBOV in Democratic Republic of Congo, 2018, emphasizing the need to develop preparedness to diagnose all filoviruses.

Objectives

The aim of this study was to optimize a new filovirus RT-qPCR to detect all filoviruses, define its limits of detection (LOD) and perform a field evaluation with outbreak samples.

Study design

A pan-filovirus RT-qPCR targeting the L gene was developed and evaluated within the EbolaMoDRAD (Ebola virus: modern approaches for developing bedside rapid diagnostics) project. Specificity and sensitivity were determined and the effect of inactivation and PCR reagents (liquid and lyophilized format) were tested.

Results

The LODs for the lyophilized pan-filovirus L-RT-qPCR assay were 9.4 copies per PCR reaction for EBOV, 9.9 for MARV, 1151 for SUDV, 65 for BDBV and 289 for Taï Forest virus. The test was set at the Pasteur Institute, Dakar, Senegal, and 83 Ebola patient samples, with viral load ranging from 5 to 5 million copies of EBOV per reaction, were screened. The results for the patient samples were in 100% concordance with the reference EBOV-specific assay.

Discussion

Overall, the assay showed good sensitivity and specificity, covered all filoviruses known to be human pathogens, performed well both in lyophilized and liquid-phase formats and with EBOV outbreak clinical samples.

1 **Keywords**

2 Ebola, Marburg, Sudan, Bundibugyo, pan-filo

3

4 **Background (2577 words)**

5 Members of marburgvirus and ebolavirus genera in the family *Filoviridae* cause highly
6 contagious illnesses with high mortality rate. There are five established species of ebolavirus:
7 Zaire (EBOV), Bundibugyo (BDBV), Sudan (SUDV), Tai Forest (TAFV) and Reston
8 (RESTV) viruses. All five can cause human infections, the first three have caused Ebola virus
9 disease (EVD) outbreaks, TAFV has been associated with only one human case, whereas
10 RESTV has been associated only with asymptomatic human seroconversions. Members of the
11 *Marburgvirus* genus, consisting of the Marburg marburgvirus (MARV) and the Ravn virus
12 (RAVV), also cause severe hemorrhagic fever in humans (Nyakarahuka et al. 2017). The third
13 genus, *Cuevavirus*, is represented by the species Lloviu cuevavirus (LLOV), which hasn't yet
14 been associated with human infections (Negredo et al. 2011). Filoviruses are thought to be
15 zoonotic, and bats are considered the likely reservoirs of these viruses (Olival et al., 2014). The
16 Egyptian fruit bat, *Rousettus aegypticus*, has been identified as the host for MARV (Towner et
17 al., 2009) while the very recently described Bombali ebolavirus (BOMV) and LLOV genome
18 sequences were discovered in samples of insectivorous bats in Africa and Europe, respectively
19 (Negredo et al., 2011; Goldstein et al., 2018). While the exact host of ebolaviruses has not been
20 confirmed yet, genetic and serological evidence of ebolavirus infections have been detected in
21 a few species of fruit bats and most recently insectivorous bats (Leroy et al., 2005; Biek et al.,
22 2006; Swanepoel et al. 2007; Laing et al., 2018; Goldstein et al., 2018). Advances in virus
23 discovery techniques have also yielded detection of novel marburg- and cuevaviruses in bats
24 in China (He et al., 2015; Yang et al., 2017) thus expanding the known range of filoviruses.

25 The largest Ebola outbreak to date took place in 2014-2016 in both rural and urban areas of
26 Guinea, Sierra Leone and Liberia in West Africa. It was caused by the EBOV, with more than
27 28 000 reported cases, including more than 11 000 deaths (World Health Organization, WHO;
28 <http://www.who.int/csr/disease/ebola/en/>). This epidemic highlighted the need for rapid
29 detection of EBOV for disease containment. In response, novel diagnostic tools have been
30 developed for rapid and safe identification of EBOV (reviewed in Clark et al., 2018). The
31 development of efficacious ring vaccination and new treatment modalities further requires
32 efficient diagnostics. Most recently, the WHO reported a new epidemic of EBOV in the
33 Democratic Republic of the Congo (DRC) in May 2018, and an unrelated outbreak some
34 2500km away in DRC in July 2018 calling for swift response yet again.

35 Between the EBOV outbreaks, a smaller outbreak of MARV occurred in Uganda in October,
36 2017, emphasizing the need to develop preparedness to diagnose all filoviruses. Whereas many
37 protocols have been developed recently for detection of EBOV, the detection methods covering
38 the whole range of filoviruses still rely largely on the protocol by Panning et al., 2007. The
39 discoveries of yet novel filoviruses (Goldstein et al. 2018) further underline the need to update
40 and improve the preparedness for rapid and sensitive detection of filoviruses.

41 Nucleic acid testing is the gold standard for filovirus diagnostics due to high viral loads that
42 become detectable in just a few days after infection (Schurtleff et al. 2015). Such diagnostic
43 tools need to be set up both at the site of the epidemic, and at sites of potential importation.
44 The EBOV outbreak in West Africa activated a broad laboratory response e.g. in Europe
45 (Reusken et al., 2018), with modern molecular diagnostics vastly available for detection of
46 EBOV. For example, freeze-dried PCR reagents would ease the transport and use of the assays
47 in harsh field conditions at the site of epidemic.

48 Critical steps in nucleic acid testing are biosafe sample preparation and transport. Different
49 protocols for the inactivation of ebolaviruses have been investigated, such as Qiagen AVL
50 buffer and the MagNa Pure Lysis buffer (MPLB; Roche Life Science, Espoo, Finland). The
51 protocol for sampling directly into MPLB has been suggested (Rosenstierne et al. 2016) and
52 this would enable biosafe transport, which is challenging nowadays. Two widely used
53 inactivators are Triton™-X 100, which interferes with lipid membranes, and lysis buffers
54 containing guanidinium thiocyanate that lyse cells and inhibit nuclease activities. Neither of
55 these can alone inactivate ebolaviruses, but parallel use of these two [e.g. Triton™-X 100
56 together with AVL buffer from Viral RNA mini kit (Qiagen) or MPLB (Roche)] have been
57 shown to fully inactivate ebolaviruses (Rosenstierne et al. 2016; Burton et al. 2017; van
58 Kampen et al. 2017). WHO has recommended the parallel usage of two different inactivation
59 reagents.

60

61 **Objectives**

62 Here we aimed to develop and evaluate a broad-range pan-filovirus detection method allowing
63 early identification of the causative agent of a filovirus outbreak. We also evaluated the freeze-
64 dried and liquid formats, and possible effects that sample inactivation methods may have on
65 the sensitivity of the assay. Finally, the method was put to test with a large panel of EVD
66 outbreak patient samples.

67

68 **Study design**

69 **Pan-filo L-RT-qPCR**

70 Two different PCR reagents; Superscript® III Platinum® One-step qRT-PCR System
71 (Invitrogen, Carlsbad, CA, USA; later referred as the Invitrogen assay) and lyophilized one-
72 step RT-qPCR reagents (Thermo Fisher Scientific, Massachusetts, USA; later referred as the
73 Thermo-lyophilized assay) were used with the same primers, probes, and viral RNA panels.

74 A pan-filo L-RT-qPCR targeting the L gene was developed and evaluated. For the assay, two
75 separate reactions were carried out for each sample in the same run.

76 In the first reaction, 160nM FAM-labelled Filo1 and Filo2 probes (adapted from Jääskeläinen
77 et al. 2015; targeting ZEBOVs) in addition to ZEBOV/MARV reverse primers [480nM of 5'-
78 AATGCATCCAATTA AAAACATTC-3' (Jääskeläinen et al. 2015), 240nM of 5'-
79 AATGCATCCARTCRAATAAATTY-3'] and 240nM ZEBOV/MARV forward primers [5'-
80 AACTGATTTAGAGAAATACAATCTTGC-3' (Jääskeläinen et al.2015), 5'-
81 CTGATCTTGAGAAATACAACCTCGC-3', 5'-
82 ACTGATYTAGAGAAATACAAYCTYGC-3'], and 160nM VIC-labelled Filo3 and Filo4
83 probes [VIC- TTT ACA CGR CAT TTC ATA GAC T-MGBNFQ and VIC- ACT GTA ATC
84 GAT GTT ATG GT-MGBNFQ; mainly targeting MARVs] were used with final
85 concentration of 2mM MgSO₄.

86 In the second reaction, a final concentration of 240nM of BDBV-RV primer [5'-
87 AATGCATCCAATTGAATAAATTT-3'], 240nM SUDV-RV [5'-
88 CATCCAATCAAAGACATTGC-3'], 320nM FILO-FW [5'-
89 ACMGACCTRGARAAATAYAACYTGCC-3'] in addition to 160nM FAM-labelled Filo5-
90 probe [FAM- ATG AGT TTA CAG CTC CAT T-MGBNFQ; mainly BDBVs] and 160nM
91 VIC-labelled Filo6 probe [VIC- TCA TCA AAT ATT GCA ACC AA-MGBNFQ; mainly
92 targeting SUDVs] were used.

93 The Invitrogen assay in the Mx3005P qPCR System (Agilent Technologies Finland Oy, Espoo,
94 Finland) was initially used to optimize the concentrations of the primers and probes. Both
95 Invitrogen and Thermo-lyophilized assays were further tested by screening of different
96 filoviruses, and to verify the specificity, and to test the PCR reagent ability to tolerate the
97 inhibition effect of Triton™-X 100 (Sigma-Aldrich, Espoo, Finland), MPLB (Roche), and
98 AVL lysis buffer (Qiagen, Hilden, Germany). Finally, the limits of detection (LODs) were
99 determined for the Thermo-lyophilized assay.

100 The RT-qPCR running protocol for Invitrogen-liquid assay was adapted from the EBOV assay
101 described in Jääskeläinen et al. (2015) and 7µl of template was used, and the protocol for
102 Thermo-lyophilized assay 3.6µl of template was used and the run was carried out as follows:
103 reverse transcription for 10 min at 45°C, PCR initial activation step for 10 min at 95°C followed
104 by 50 cycles of denaturation for 15s at 95°C, and annealing and extension for 70s at 60°C.

105

106 **Viral controls**

107 Quantified *in vitro* RNAs were produced using constructs for EBOV and MARV L genes
108 (described in Jääskeläinen et al. 2015), in addition to synthesized L-gene constructs of SUDV
109 and BDBV ebolaviruses (GeneArt™ Plasmid Construction Service, Thermo Fischer
110 Scientific). RNAs from inactivated whole virus controls of EBOV/Guinea C05 and
111 EBOV/Mayinga, MARV/Angola, RAVV, SUDV/Boniface, BDBV/E76, TAFV/Ivory Coast
112 and RESTV were obtained from Public Health England (PHE, Porton Down, Salisbury, UK).
113 These viruses were cultivated in Vero E6 cells, inactivated, and RNA extracted using QIAamp
114 Viral RNA Mini kit (Qiagen, Hilden, Germany) according to manufacturer's instruction.

115

116 **Specificity and inhibition tests**

117 For assessing specificity, EDTA-blood samples from 45 individuals that were sent for routine
118 human herpesvirus 6 nucleic acid testing (later referred as HU-samples) in Helsinki University
119 Hospital (HUSLAB, Helsinki, Finland; anonymous samples, research permit TYH2017257),
120 were extracted using MagNa Pure 96 automated system and nucleic acid kits (MPLB lysis;
121 Roche Life Science, Espoo, Finland), and tested using the Invitrogen and Thermo-lyophilized
122 assays. In addition, for testing other viral hemorrhagic fever agents, the RNAs from inactivated
123 whole virus controls of Lassa virus (strain Liberia; LASV), Dengueviruses 1-4 (DENV1-4),
124 Yellow fever virus (strain 17D; YFV), Rift Valley fever virus (strain RKI; RVFV) and
125 Crimean-Congo hemorrhagic virus (strain Hoti; CCHFV) were extracted using QIAamp Viral
126 RNA Mini kit (Qiagen) (Table 1).

127 For Triton™-X 100 (Sigma-Aldrich, Espoo, Finland) inhibition tests, excess amount of
128 Triton™-X 100 was added to EDTA-blood samples in final volume of 10% in order to test any
129 PCR inhibition effect due to the reagent in both Invitrogen and Thermo-lyophilized assays.
130 Triton-treated (10 min at room temperature) EDTA-blood samples were extracted using AVL
131 and QIAamp Viral RNA Mini kit (Qiagen). In addition, EDTA-blood samples without extra
132 Triton treatment were extracted using MPLB and MagNA Pure extraction system (Roche).
133 Different amounts of EBOV, MARV, SUDV or BDBV RNAs were spiked in the extracted
134 samples, and both Thermo-lyophilized and Invitrogen assays were carried out (Figure 1).

135

136 **Sensitivity**

137 Sensitivity of the pan-filo L-RT-qPCR was tested using the Thermo-lyophilized assay and
138 serial dilutions of quantified RNA transcripts (Qubit, Thermo Fisher Scientific) of EBOV,
139 MARV, SUDV and BDBV L-gene, and TAFV (PHE, quantified). Five parallel reactions and
140 Probit Regression (SPSS, IBM) were used to determine LODs. The Invitrogen assay was tested

141 in parallel with the WHO-approved RealStar® Filovirus RT-PCR Kit (Altona Diagnostics
142 GmbH, Hamburg, Germany) using ZEBOV strain Guinea (range 5-1000 genome copies/PCR
143 reaction; PHE), SUDV L-gene RNA (range 7-1.5E6 genome copies/PCR reaction) and BDBV
144 L-gene RNA (range 13-1.25E6 genome copies/PCR reaction) (Table 1). In addition, whole
145 virus controls (Table 1, PHE) were tested to screen different filovirus targets.

146

147 **Screening of Ebola patient samples**

148 Samples were collected in Guinea between December 2014 and May 2015 as part of the
149 Institute Pasteur de Dakar (IPD) diagnostics activities of suspected EVD cases (under an
150 emergency response mandate from the government of Guinea and WHO, ref
151 0235/14/GUI/CPC; all patients agreed to be tested for Ebola virus infection and leftover
152 samples to be used for further investigations). Suspect Ebola patients were defined as any
153 person with recent or past sudden onset of fever and having been in contact with a suspected,
154 probable or confirmed case of EVD, or any person with sudden onset of fever and at least three
155 of the following symptoms: headaches, anorexia/loss of appetite, lethargy, myalgia, arthralgia,
156 breathing difficulties, or any person with inexplicable bleeding. Eighty-three serum samples
157 from acute cases were extracted using QIAamp Viral RNA Mini kit (Qiagen) according to
158 manufacturer's instructions in IPD, Senegal. These were all EBOV nucleic acid positive using
159 the reference EBOV NP-RT-qPCR (Weidmann et al. 2004; using modified forward primer of
160 5'-ATGATGGARGCTACGGCG-3' and probe 5'-CARAGTTACTCGGAAAACGGCAT)
161 with viral loads ranging from 5 RNA copies to 5.5 million RNA copies per reaction. In IPD,
162 the pan-filo L-RT-qPCR and EBOV NP-RT-qPCR were carried out in parallel using
163 QuantiTect® Probe RT-PCR kit (Qiagen) and 5µl of template for performance comparison.

164

165 **Results**

166 Both Invitrogen and Thermo-lyophilized pan-filo L-RT-qPCR assays tested negative for HU-
167 samples ($N=45$), as well as for LASV, DENV1-4, YFV, RVFV and CCHFV, indicating
168 analytical specificity of 100% (95CI: 94.8-100%; Table 1). In addition, both assays detected
169 EBOV/Guinea C05, EBOV/Mayinga, MARV/Angola, RAVV, SUDV/Boniface, BDBV/E76,
170 TAFV/Ivory Coast and RESTV (Table 1).

171 The LODs (SPSS, Probit, 95CI) for Thermo-lyophilized assay were 9.9 copies/PCR reaction
172 for MARV, 9.4 for EBOV, 65 for BDBV, 1151 for SUDV and 289 for TAFV (PHE).

173 The Invitrogen pan-filo L-RT-qPCR assay was as good as the RealStar® Filovirus Screen RT-
174 PCR Kit for EBOV, however, for BDBV and SUDV samples there were minor differences
175 (Table 1).

176 Triton™-X 100 (Sigma-Aldrich), AVL (Qiagen) or MPLB (Roche) did not interfere the
177 Invitrogen or Thermo-lyophilized one-step assays (Figure 1).

178 All of the patient samples tested (83) from IPD (Senegal) were positive for EBOV nucleic acids
179 using our pan-filo L-RT-qPCR assay and EBOV NP-RT-qPCR (Figure 2) indicating 100%
180 analytical sensitivity. The LOD for EBOV NP-RT-qPCR was 4 copies/PCR reaction (tested in
181 University of Helsinki; SPSS, Probit, 95CI).

182

183 **Discussion**

184 Filoviruses were first isolated more than 50 years ago, and outbreaks with high mortality have
185 subsequently been caused by four viruses, MARV (9 times) SUDV (5 times), BDBV (twice)
186 and EBOV (14 times) (WHO). For containing and restricting the epidemics, including
187 establishing control measures and therapeutics, accessible, rapid and reliable diagnostic tests

188 are essential. IgM and IgG detection assays are used to confirm resolved disease or to
189 diagnostically monitor samples of cases beyond the diagnostic window for molecular detection.
190 While rapid antigen detection tests with varying sensitivity and specificity have been developed
191 for EBOV detection [Walker et al., 2015; Broadhurst et al. 2015], nucleic acid detection
192 remains the cornerstone of diagnostics. It is a challenge to find simple protocols, particularly
193 primer and probe sequences applicable to all pathogenic filoviruses, yet tests covering all
194 filoviruses would be essential in early identification of outbreaks as well as occasional cases in
195 endemic regions or travelers. Adding such a test and its evaluation is what we report here.
196 However, in future, the lyophilized protocol would benefit from lyophilized primers and probes
197 in mastermixes making the protocol more suitable for field conditions.

198

199 After the West African EBOV epidemic, a variety of methods, inactivation protocols and
200 handling procedures have been studied (Rosenstierne et al. 2016; Burton et al. 2017; van
201 Kampen et al. 2017). Most of the detection methods, however, have been based on the detection
202 of only EBOV nucleic acids, and this limitation can cost time for diagnosis of other filoviruses.
203 At the moment there is only one commercial pan-filovirus kit (RealStar® Filovirus Screen RT-
204 PCR Kit) approved by WHO that also detects MARV, others still aim to detect EBOV antigen
205 or nucleic acids (WHO; [http://www.who.int/medicines/ebola-
206 treatment/emp Ebola_diagnostics/en/](http://www.who.int/medicines/ebola-treatment/emp Ebola_diagnostics/en/)). These WHO-approved tests include Liferiver™ Ebola
207 Virus (EBOV) Real Time RT-PCR kit (Shanghai ZJ BioTech Co., Ltd) which can be used for
208 detection EBOV, SUDV, TAFV, BDBV, and Xpert® Ebola Test (Cepheid AB, Sweden),
209 FilmArray™ Biothreat-E (BioFire Defence LLC, USA) which both only detect EBOV.

210 The 2-well pan-filo L-RT-qPCR assay described here detected all the tested strains of MARV,
211 EBOV, BDBV, SUDV, TAFV, as well as RESTV. In addition, we were able to validate the

212 pan-filo L-RT-qPCR assay with clinical samples from the West-African EBOV outbreak with
213 excellent performance. Overall, the assay achieved better performance for EBOV and MARV
214 than rest of the tested targets, but was still at the same level as WHO-approved RealStar®
215 Filovirus Screen RT-PCR kit. With this in mind, it's recommended to test several samples from
216 patient suspected for VHF to avoid false negative results at the early onset of disease.

217 The specificity was 100%, and the lyophilized or liquid assays were not affected by common
218 chemical inactivation reagents, *i.e.* MPLB, AVL or Triton™-X 100. These results are in line
219 with Rosenstierne et al. (2016) who tested MPLB and AVL buffers.

220 Based on the sequences, the pan-filo L-RT-qPCR primers and probes are not a perfect match
221 for BOMV (MF319185; forward primer 4, reverse 2, and VIC-probe 3 mismatches) or other
222 bat-related filoviruses in GenBank (National Center for Biotechnology Information, USA).
223 However, when screening Kenyan bat samples, with the pan-filo L-RT-qPCR we detected one
224 sample positive for filovirus. The bat-related filovirus was later sequenced and identified as
225 BOMV (Forbes et al., Emerging Infectious Diseases 2019, in press).

226 We conclude that the developed assays, both lyophilized and liquid phase, can be used
227 effectively to screen samples from patients suspected for any known filoviral hemorrhagic
228 fever, and both marburg and ebolaviruses can be detected.

229

230 **Acknowledgements**

231 We thank the Robert Koch-Institut in Berlin, Germany, for providing the viral standard
232 preparations (DENV, YFV, CCHFV, LASV) for diagnostic purposes. We thank HUSLAB
233 PCR team personnel, Johanna Martikainen (University of Helsinki) and Minttu Kaloinen
234 (University of Helsinki) for technical assistance.

235 **Funding**

236 This project is part of the EbolaMoDRAD (Ebola virus: modern approaches for developing
237 bedside rapid diagnostics) consortium, which has received funding from the Innovative
238 Medicine Initiative 2 Joint Undertaking under grant agreement N°115843. This Joint
239 Undertaking receives support from the European Union's Horizon 2020 research and
240 innovation programme and EFPIA. This work was also funded by Helsinki University Hospital
241 (HUSLAB; research permit TYH2017257).

242

243 **Conflict of Interest**

244 There are no conflicts of interest.

245

246

247 **References**

248

249 **Biek R**, Walsh PD, Leroy EM, Real LA. Recent common ancestry of Ebola Zaire virus found
250 in a bat reservoir. *PLoS Pathog.* 2006 2:e90.

251

252 **Broadhurst MJ**, Kelly JD, Miller A, Semper A, Bailey D, Groppelli E, Simpson A, Brooks T,
253 Hula S, Nyoni W, Sankoh AB, Kanu S, Jalloh A, Ton Q, Sarchet N, George P, Perkins MD,
254 Wonderly B, Murray M, Pollock NR. ReEBOV Antigen Rapid Test kit for point-of-care and
255 laboratory-based testing for Ebola virus disease: a field validation study. *Lancet* 2015 386:867-
256 874.

257

258 **Burton JE**, Easterbrook L, Pitman J, Anderson D, Roddy S, Bailey D, Vipond R, Bruce CB,
259 Roberts AD. The effect of a non-denaturing detergent and a guanidinium-based inactivation
260 agent on the viability of Ebola virus in mock clinical serum samples. *J Virol Methods.* 2017
261 250:34-40.

262

263 **Clark DJ**, Tyson J, Sails AD, Krishna S, Staines HM. The current landscape of nucleic acid
264 tests for filovirus detection. *J Clin Virol.* 2018 103:27-36.

265

266 **Coarsey CT**, Esiobu N, Narayanan R, Pavlovic M, Shafiee H, Asghar W. Strategies in Ebola
267 virus disease (EVD) diagnostics at the point of care. *Crit Rev Microbiol.* 2017 43:779-798.

268

269 **Forbes** KM, Webala PW, Jääskeläinen AJ, Abdurahman S, Ogola J, Masika MM, Kivistö I,
270 Alburkat H, Plyusnin I, Levanov L, Korhonen EM, Huhtamo E, Mwaengo D, Smura T,
271 Mirazimi A, Anzala O, Olli Vapalahti O, Sironen T. Bombali ebolavirus is widespread in
272 Africa: evidence from an infected *Mops condylurus* bat in south-east Kenya. Manuscript.
273

274 **Goldstein** T, Anthony SJ, Gbakima A, Bird BH, Bangura J, Tremeau-Bravard A, Belaganahalli
275 MN, Wells HL, Dhanota JK, Liang E, Grodus M, Jangra RK, DeJesus VA, Lasso G, Smith
276 BR, Jambai A, Kamara BO, Kamara S, Bangura W, Monagin C, Shapira S, Johnson CK,
277 Saylor K, Rubin EM, Chandran K, Lipkin WI, Mazet JAK. The discovery of Bombali virus
278 adds further support for bats as hosts of ebolaviruses. *Nat Microbiol.* 2018 3:1084-1089. .
279 Erratum in: *Nat Microbiol.* 2018 3:1486.
280

281 **He** B, Feng Y, Zhang H, Xu L, Yang W, Zhang Y, Li X, Tu C. Filovirus RNA in Fruit Bats,
282 China. *Emerg Infect Dis.* 2015 21:1675-1677.
283

284 **Jääskeläinen** AJ, Moilanen K, Aaltonen K, Putkuri N, Sironen T, Kallio-Kokko H, Vapalahti
285 O. Development and evaluation of a real-time EBOV-L-RT-qPCR for detection of Zaire
286 ebolavirus. *J Clin Virol.* 2015 67:56-58.
287

288 **Laing** ED, Mendenhall IH, Linster M, Low DHW, Chen Y, Yan L, Sterling SL, Borthwick S,
289 Neves ES, Lim JSL, Skiles M, Lee BPY, Wang LF, Broder CC, Smith GJD. Serologic
290 Evidence of Fruit Bat Exposure to Filoviruses, Singapore, 2011-2016. *Emerg Infect Dis.* 2018
291 24:114-117.

292

293 **Leroy EM**, Kumulungui B, Pourrut X, Rouquet P, Hassanin A, Yaba P, Délicat A, Paweska
294 JT, Gonzalez JP, Swanepoel R. Fruit bats as reservoirs of Ebola virus. *Nature*. 2005 38:575-
295 576.

296

297 **Mulangu S**, Alfonso VH, Hoff NA, Doshi RH, Mulembakani P, Kisalu NK, Okitolonda-
298 Wemakoy E, Kebela BI, Marcus H, Shiloach J, Phue JN, Wright LL, Muyembe-Tamfum JJ,
299 Sullivan NJ, Rimoin AW. Serologic Evidence of Ebolavirus Infection in a Population With
300 No History of Outbreaks in the Democratic Republic of the Congo. *J Infect Dis*. 2018
301 217:529-537.

302

303 **Negredo A**, Palacios G, Vázquez-Morón S, González F, Dopazo H, Molero F, Juste J, Quetglas
304 J, Savji N, de la Cruz Martínez M, Herrera JE, Pizarro M, Hutchison SK, Echevarría JE, Lipkin
305 WI, Tenorio A. Discovery of an ebolavirus-like filovirus in europe.
306 *PLoS Pathog*. 2011 7:e1002304.

307

308 **Nyakarahuka L**, Ojwang J, Tumusiime A, Balinandi S, Whitmer S, Kyazze S, Kasozi S,
309 Wetaka M, Makumbi I, Dahlke M, Borchert J, Lutwama J, Ströher U, Rollin PE, Nichol ST,
310 Shoemaker TR. Isolated Case of Marburg Virus Disease, Kampala, Uganda, 2014. *Emerg*
311 *Infect Dis*. 2017 23:1001-1004.

312

313 **Olival** KJ, Hayman DTS. Filoviruses in bats: current knowledge and future directions. *Viruses*.
314 2014 6:1759–1788.

315

316 **Panning** M, Laue T, Olschlager S, Eickmann M, Becker S, Raith S, Courbot MC, Nilsson M,
317 Gopal R, Lundkvist A, di Caro A, Brown D, Meyer H, Lloyd G, Kummerer BM, Gunther S,
318 Drosten C. Diagnostic reverse-transcription polymerase chain reaction kit for filoviruses based
319 on the strain collections of all European biosafety level 4 laboratories. *J Infect Dis*. 2007 196
320 Suppl 2:S199-204.

321

322 **Reusken** CB, Mögling R, Smit PW, Grunow R, Ippolito G, Di Caro A, Koopmans M. Status,
323 quality and specific needs of Ebola virus diagnostic capacity and capability in laboratories of
324 the two European preparedness laboratory networks EMERGE and EVD-LabNet. *Euro*
325 *Surveill*. 2018 23(19).

326

327 **Rosenstierne** MW, Karlberg H, Bragstad K, Lindegren G, Stoltz ML, Salata C, Kran AM,
328 Dudman SG, Mirazimi A, Fomsgaard A. Rapid Bedside Inactivation of Ebola Virus for Safe
329 Nucleic Acid Tests. *J Clin Microbiol*. 2016 54:2521-2529.

330

331 **Shurtleff** AC, Whitehouse CA, Ward MD, Cazares LH, Bavari S. Pre-symptomatic diagnosis
332 and treatment of filovirus diseases. *Front Microbiol*. 2015 6:108.

333

334 **Swanepoel R**, Smit SB, Rollin PE, Formenty P, Leman PA, Kemp A, Burt FJ, Grobbelaar AA,
335 Croft J, Bausch DG, Zeller H, Leirs H, Braack LE, Libande ML, Zaki S, Nichol ST, Ksiazek
336 TG, Paweska JT; International Scientific and Technical Committee for Marburg Hemorrhagic
337 Fever Control in the Democratic Republic of Congo. Studies of reservoir hosts for Marburg
338 virus. *Emerg Infect Dis.* 2007 13:1847-1851.

339

340 **Towner JS**, Amman BR, Sealy TK, Carroll SA, Comer JA, Kemp A, Swanepoel R, Paddock
341 CD, Balinandi S, Khristova ML, Formenty PB, Albarino CG, Miller DM, Reed ZD, Kayiwa
342 JT, Mills JN, Cannon DL, Greer PW, Byaruhanga E, Farnon EC, Atimnedi P, Okware S,
343 Katongole-Mbidde E, Downing R, Tappero JW, Zaki SR, Ksiazek TG, Nichol ST, Rollin PE.
344 Isolation of genetically diverse Marburg viruses from Egyptian fruit bats. *PLoS Pathog.* 2009
345 5:e1000536.

346

347 **van Kampen JJA**, Tintu A, Russcher H, Fraaij PLA, Reusken CBEM, Rijken M, van
348 Hellemond JJ, van Genderen PJJ, Koelewijn R, de Jong MD, Haddock E, Fischer RJ, Munster
349 VJ, Koopmans MPG. Ebola Virus Inactivation by Detergents Is Annulled in Serum. *J Infect*
350 *Dis.* 2017 216:859-866.

351

352 **Weidmann M**, Mühlberger E, Hufert FT. Rapid detection protocol for filoviruses. *J Clin Virol.*
353 2004 30:94-99.

354

355 **Walker NF**, Brown CS, Youkee D, Baker P, Williams N, Kalawa A, Russell K, Samba AF,
356 Bentley N, Koroma F, King MB, Parker BE, Thompson M, Boyles T, Healey B, Kargbo B,

357 Bash-Taqi D, Simpson AJ, Kamara A, Kamara TB, Lado M, Johnson O, Brooks T. Evaluation
358 of a point-of-care blood test for identification of Ebola virus disease at Ebola holding units,
359 Western Area, Sierra Leone, January to February 2015. *Euro Surveill.* 2015 20(12).

360

361 **Yang** XL, Zhang YZ, Jiang RD, Guo H, Zhang W, Li B, Wang N, Wang L, Waruhiu C, Zhou
362 JH, Li SY, Daszak P, Wang LF, Shi ZL. Genetically Diverse Filoviruses in Rousettus and
363 Eonycteris spp. Bats, China, 2009 and 2015. *Emerg Infect Dis.* 2017 23:482-486.

364

365

Figure 1a and b. Comparing the performance of the pan-filo L-RT-qPCR using Thermo-lyophilized and Invitrogen-liquid assays for potential inhibitory effects of different reagents and inactivation methods [Fig 1a., Triton™-X 100 treatment (Triton) or Fig 1b. Magna Pure Lysis buffer (MPLB)].

Fig. 1a


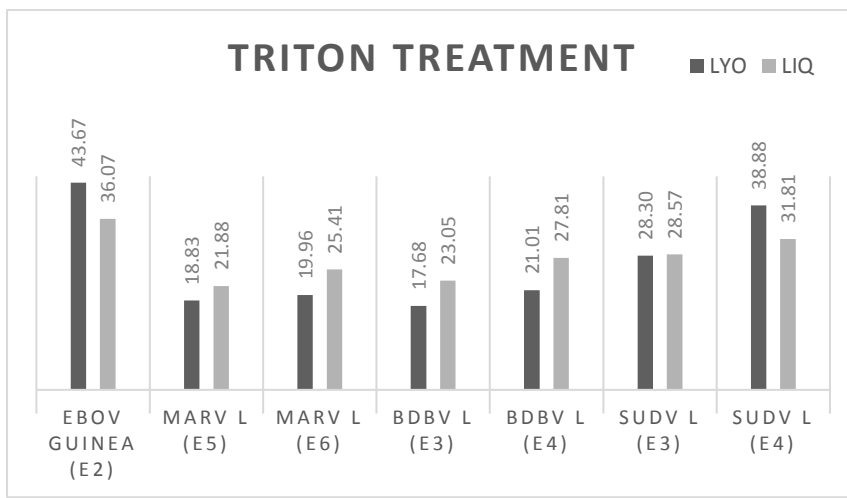


Fig. 1b

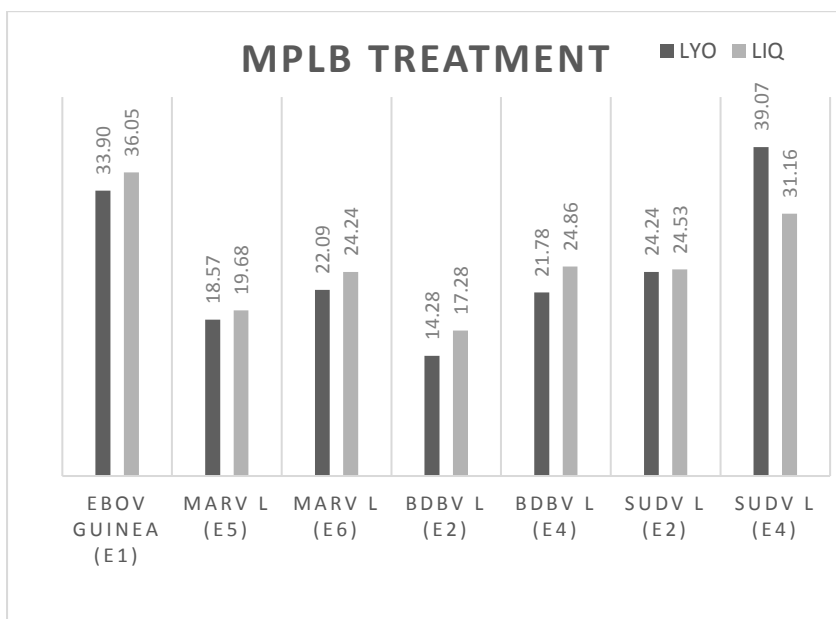

Ex, 10^{-x} ($E1=10^{-1}$, $E2=10^{-2}$...) dilution, single replicate; MARV L, L gene construct of Marburg virus; ZEBOV Guinea, RNA extract of Zaire ebolavirus; BDBV L, L gene construct of Bundibugyo virus; SUDV L, L gene construct of Sudan ebolavirus; negat, negative.

Triton: EDTA-blood TritonTM-X 100 treated and extracted using Qiagen kit, spiked with filoviral RNA

MPLB: EDTA-blood, Magna Pure LC extracted, using Magna Pure Lysis buffer, spiked with filoviral RNA

Over Ct 40 results are not considered real positive until confirmed by another test if used in diagnosis of filoviral disease in clinical settings. Here Ct-values are listed due to the comparison purposes.

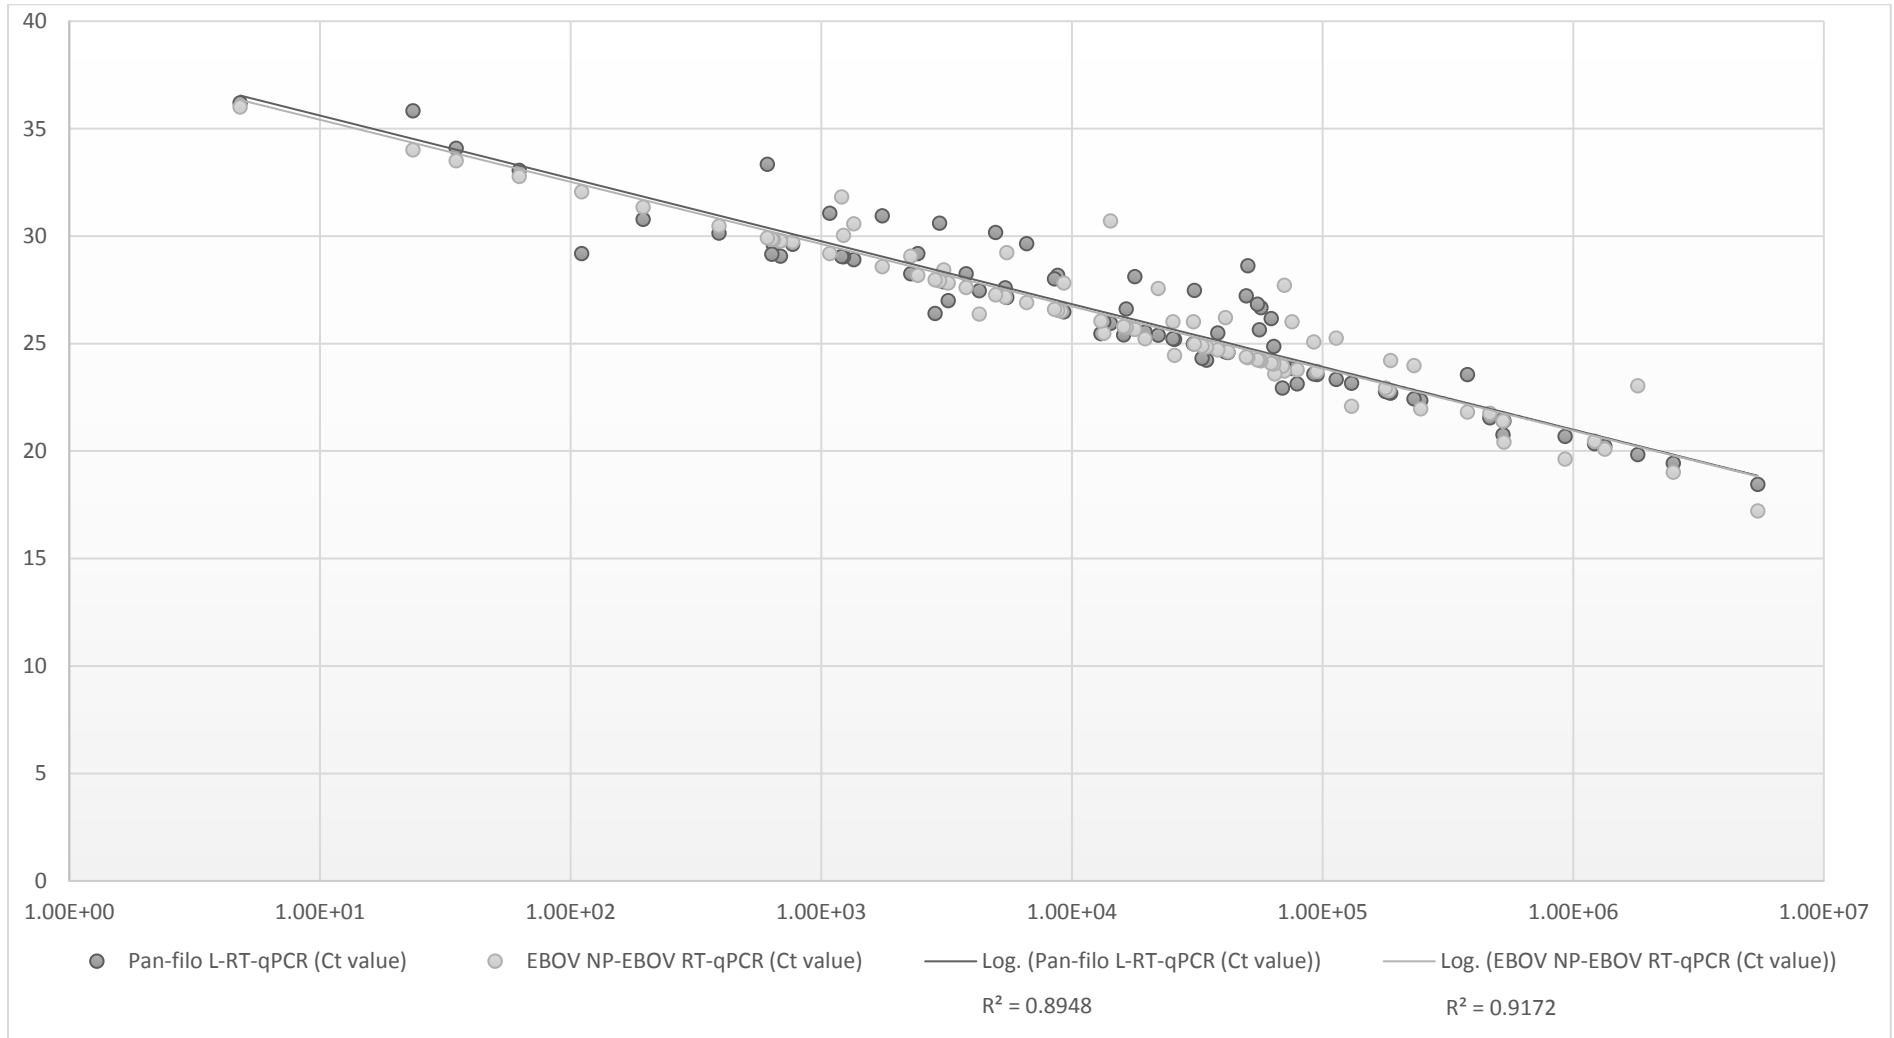


Figure 2. Parallel results of pan-filo L-Rt-qPCR (this study) and EBOV NP-RT-qPCR (Weidmann et al. 2004) assays. The RNA copy numbers (5 copies to 5.5 million copies) of EVD patient samples are presented in the X-axis (logarithmic scale, \log_{10}) and Ct values in the Y-axis. R^2 , R-squared.

Panel/sample material	Microbial agent	No of samples/tests, neg/pos		Pan-filo L-RT-qPCR assays: Results from Liquid and Lyophilized platforms compared			
		neg for FILO RNA	pos for FILO RNA	neg for FILO RNA		pos for FILO RNA	
				Liq (Invitrogen)	Lyo (Thermo)	Liq (Invitrogen)	Lyo (Thermo)
NEG: Whole blood ¹	Negative sample panel	45	-	45/45	45/45	0/45	0/45
	Total	45	-	45/45	45/45	0/45	0/45
NEG: Viruses ²	YFV (strains 17D)	3	-	3/3	3/3	0/3	0/3
	DENV1 (RKI)	3	-	3/3	3/3	0/3	0/3
	DENV2 (RKI)	3	-	3/3	3/3	0/3	0/3
	DENV3 (RKI)	3	-	3/3	3/3	0/3	0/3
	DENV4 (RKI)	3	-	3/3	3/3	0/3	0/3
	LASV (strain Liberia, RKI)	3	-	3/3	3/3	0/3	0/3
	RVFV (strain RKI, RKI)	3	-	3/3	3/3	0/3	0/3
	CCHFV (strain Hoti, RKI)	3	-	3/3	3/3	0/3	0/3
	Total	24	-	24/24	24/24	0/24	0/24
All FILO negatives		69/69 (100%; 95CI 94.8-100%)					
POS: Viruses/Viral RNAs	ZEBOV (strain Mayinga, PHE)	-	3	0/3	0/3	3/3	3/3
	MARV (strain Angola)	-	2	0/2	0/2	2/2	2/2
	MARV (strain Ravn)	-	2	0/2	0/2	2/2	2/2
	SUDV strain Boniface	-	2	0/2	0/2	2/2	2/2
	BDBV strain E76	-	2	0/2	0/2	2/2	2/2
	Tai Forest virus strain Ivory Coast*	-	2	0/2	0/2	2/2	2/2
	Reston virus	-	2	0/2	0/2	2/2	2/2
	MARV L-gene RNA (HU)*	-	15	0/15	0/15	15/15	15/15

	ZEBOV L-gene construct RNA (HU)	-	15	0/15	0/15	15/15	15/15
	Total	-	45	0/45	0/45	45/45	45/45
POS: 38 viral controls tested using RealStar® Filovirus RT- PCR Kit³ and Invitrogen assay	Virus	Reference test: RealStar® Filovirus 5 parallel rxns, mean Ct (±SD)				Liq, Invitrogen 5 parallel rxns, mean Ct (±SD)	
	ZEBOV (strain Guinea, PHE)*; 100 copies/rxn	5/5, Ct 30.3 (±0.31)				5/5, Ct 35.6 (±0.66)	
	50 copies/rxn	5/5, Ct 32.3, (±2.7)				4/5, Ct 36.2 (±0.9)	
	25 copies/rxn	1/5, Ct 34.3 (ND)				1/5, Ct 36.1 (ND)	
	Total ZEBOV	11/15				10/15	
	SUDV L-gene (GeneArt), 1500 copies/rxn	5/5, Ct 31.3 (±3.5)				5/5, Ct 38.3 (±1.3)	
	150 copies/rxn	2/5, Ct 33.7 (±3.8)				1/5, Ct 38.8 (ND)	
	15 copies/rxn	0/5				0/5	
	Total SUDV	7/15				6/15	
	BDBV L-gene (GeneArt)**, 1250; 625; 125 copies/rxn	1250: Ct 31.4 (ND); 625: Ct 32.0 (ND); 125:Ct 35.4 (ND)				1250: Ct 33.4 (ND), 625: Ct 36.5 (ND), 125: Ct 36.3 (ND)	
	62.5 copies/rxn	1/5, Ct 30 (ND)				4/5, Ct 38.1 (±1.4)	
	Total BDBV	4/8				7/8	
	Altogether	22/38				23/38	

Table 1. Sample panels, materials and viruses used for validation of both liquid and lyophilized assay formats of the pan-filo L-RT-qPCR, and the results of the validation.

POS, positive; NEG, negative; FILO, filoviruses; rxn, reaction; ND, not determined; ZEBOV, Zaire ebolavirus; MARV, Marburg virus; BDBV, Bundibugyo virus; SUDV, Sudan ebolavirus; HU, University of Helsinki; PHE, Public Health England; RKI, Robert Koch Institute; DENV,

denguevirus; LASV, Lassa virus; YFV, yellow fever virus; CCHFV, Crimean-Congo Hemorrhagic virus; RVFV, Rift-Valley Fever virus.

** Only one reaction was carried out.

¹EDTA-Blood samples (Helsinki University Hospital, HUSLAB, Finland)

²RNA extractions from inactivated virus cultivations kindly provided by Prof. Niedrig (Robert Koch Institute, Germany).

³ RealStar® Filovirus Screen RT-PCR Kit (Altona Diagnostics GmbH, Hamburg, Germany). Only liquid phase Invitrogen pan-filo L RT-qPCR assay was carried out parallel with RealStar® Filovirus Screen RT-PCR Kit.